



PhoenixTM
Phoenix Temperature Measurement

Where experience counts!!

Thermal View Survey - PhoenixTM

File Telemetry Edit Options Help

PhoenixTM

Run a Survey
New Survey
Download
Settings
Standard Settings
TUS Levels
TUS Frames
TC Correction
Logger Correction
Analysis
TUS Profiles
Temperature Data
TUS Results
View Frame
Reporting
Print TUS Report
Help
User Manual

Temperature Profile

Thermocouple Locations

TUS Levels

Survey Name or Specification: PhoenixTM Oven 175_250 +/-15

Survey Level °C	Tolerance + °C	Tolerance - °C	Stabilization Time (HH:MM)	Survey Time (HH:MM)
175.0	15.0	15.0	00:15	00:30
250.0	15.0	15.0	00:15	00:30

PTM1210

PhoenixTM

PTM4220 Delta

V5.2

Thermal View Survey Analysis Software

PhoenixTM 'Thermal View Survey' is a powerful software package for recording and analysing TUS data from your furnace and oven surveys. The software is compatible with the complete PhoenixTM data logger range. Whether performing the TUS thru-process employing the travelling PTM1200 data logger protected within the appropriate thermal barrier for semi-continuous or continuous heat treat processes or stand-alone PTM4200 data logger for batch furnaces the software allows complete data logger set-up, real time data monitoring and full TUS analysis and reporting. The software has been developed to comply with all the necessary analysis and reporting requirements of AMS2750G or CQI-9 TUS pyrometry standards. Fully traceable and certified TUS reports can be easily and efficiently generated saving production time and freeing up your technical staff.

Remote Data Logger Control & Monitoring

Wireless (Bluetooth and RF*) set-up and control of data logger and live monitoring of data against TUS tolerances at each sequential TUS temperature level. Collect TUS data with confidence and efficiency that you know will comply.

Efficient Quick TUS Parameter Set-up

Create template files for key TUS parameters including TUS frame set-up, TUS tolerance levels and data logger and thermocouple correction factor files allowing error free quick routine TUS operation without repeat manual parameter set-up.

Accurate Analysis and Compliant Reporting

Customised TUS analysis tools to analyse survey data accurately with automatically applied correction factors. Report generator tool allows configuration of TUS report to comply fully with AMS2750G or CQI-9.

* Option with data logger


Software Power

- Full data logger reset and control
- Real time analysis either via USB cable, Bluetooth, or optional RF Telemetry
- TUS with up to 60 thermocouples (Merging 3 x 20 channel TUS runs)
- Data logger and Thermocouple correction factor files accurately generated across entire measurement range.
- Correction Factors applied automatically to complete TUS data.
- Full temperature data at TUS levels with pass/fail colour coding
- Full zoom control of graphical data
- Temperature overshoot warnings
- TUS temperature level library
- TUS zone fitting to temperature data
- TUS frame library & on-screen view
- Furnace class result at each level
- Rounding Up/Down to ASTM E29 and IEC 80000-1
- On screen notes
- User customised printed report designed to meet ASM2750G requirements
- Export to CSV file
- Import Furnace Control TC data
- On screen help
- Database storage
- Password protection
- Audit trail




Key Screens & Functions


Key Features of the Thermal View Survey Software providing an accurate, quick and efficient TUS reporting facility.

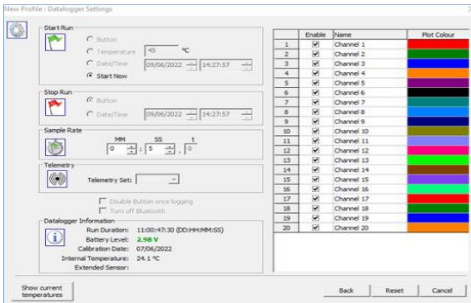


Full Data Logger Status, Set-up and Control (including TUS sample interval, channel configuration)

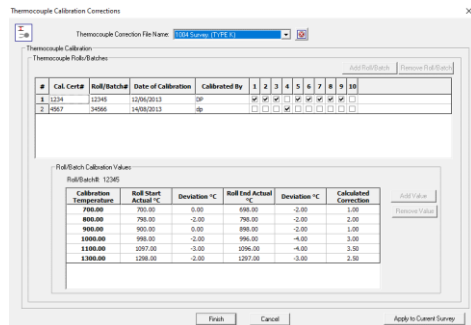

Thermocouple calibration files allowing accurate set-up of TC correction factors across entire temperature range. Not just at single temperature.

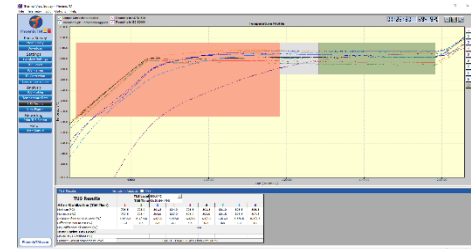


Full graphical and analysis reporting of TUS levels showing full overshoot search, stabilise and TUS time phases.

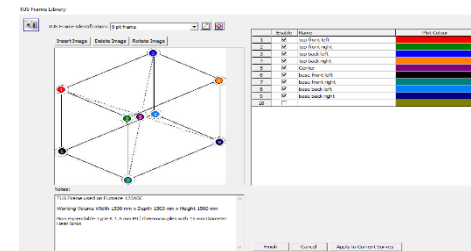


TUS frame Library files allowing clear documentation of TUS thermocouple location on TUS frame within furnace working volume.

Note: All Products are continually improved, specifications may be changed without prior notice. Ref: PhoenixTM_Datasheet_SW25_10.3_UK 20220707


Represented by:

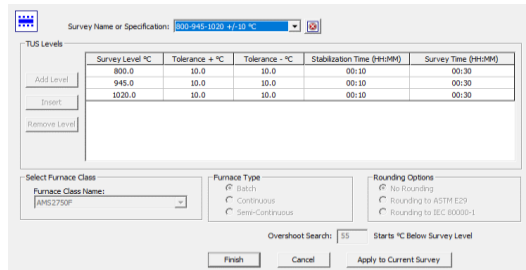


TUS level library files allowing comprehensive set-up of temperatures, times, rounding and furnace class settings.

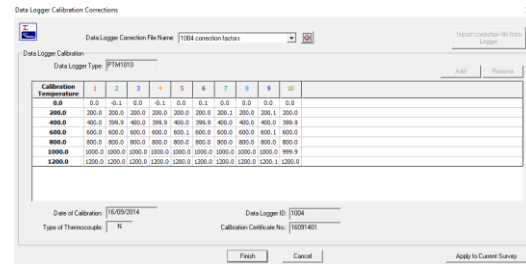

Data logger correction file read directly from field test instrument permitting automatic TUS correction and certified documentation.

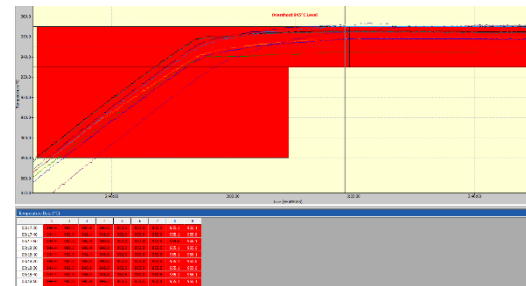

Clear reporting of overshoot errors both graphically and in raw data highlighting exactly where TUS failure occurred.

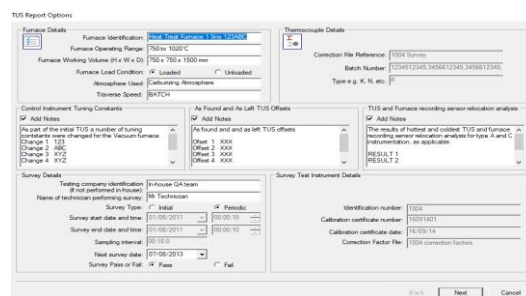

TUS report dialogue allowing customisable set-up of all information (auto and manual input) required for AMS2750G and CQI-9 report generation.

www.phoenixtm.com

www.phoenixtm.de



PhoenixTM LLC. 4600 140th Avenue North, Suite 180, Clearwater, FL 33762 USA
Tel: +1(727)608 4314 info@phoenixtm.com



PhoenixTM Ltd. 25 Earith Business Park Meadow Drive, Earith, Cambridgeshire PE28 3QF, UK
Tel: +44 (0) 1353 223100 sales@phoenixtm.com



PhoenixTM GmbH Dehmer Str 48 32549 Bad Oeynhausen, Germany
Tel: +49 5731 300280 0 info@phoenixtm.de